



PT.AVERON

— GLOBAL INDONESIA —

IMPORTER & SUPPLIER OF MEDICAL INSTRUMENTS



**Electro
Surgical**

 www.averonindonesia.com

Diathermy/ Bipolar

Diathermy Scissors

Diathermy Forceps

Bipolar Forceps


Handles, Needles and Blades

Leads

Quivers

Diathermy Scissors and Forceps

Turner Warwick Diathermy Scissors

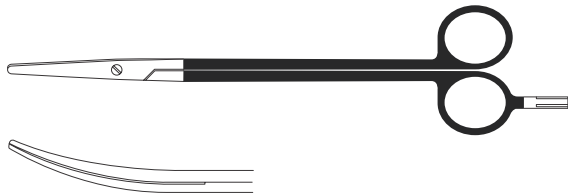

Straight


Code	Description
PA-DIA/072	190mm long
PA-DIA/073	230mm long
PA-DIA/074	250mm long

Curved

Code	Description
PA-DIA/075	190mm long
PA-DIA/076	230mm long
PA-DIA/077	250mm long


Riches Artery Forceps

Screw joint, curved

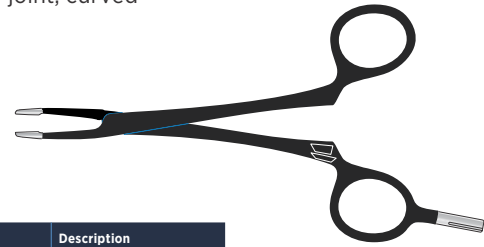

Code	Description
PA-DIA/014	127mm long
PA-DIA/015	152mm long
PA-DIA/016	178mm long
PA-DIA/017	185mm long
PA-DIA/018	228mm long

Adson Forceps

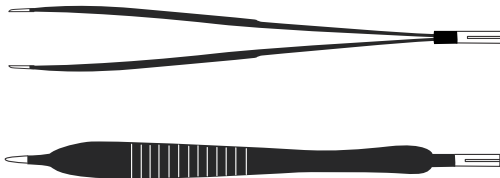

Code	Description
PA-DIA/003	152mm long

Dissecting Forceps




Serrated

Code	Description
PA-DIA/004	152mm long
PA-DIA/005	178mm long
PA-DIA/006	203mm long
PA-DIA/007	228mm long
PA-DIA/008	254mm long

1-2 teeth

Code	Description
PA-DIA/009	152mm long
PA-DIA/010	178mm long
PA-DIA/011	203mm long
PA-DIA/012	228mm long
PA-DIA/013	254mm long

Wilson Hey Artery Forceps

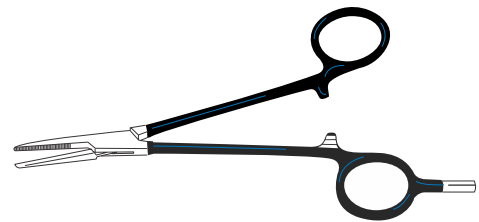

Straight

Code	Description
PA-DIA/023	152mm long
PA-DIA/024	178mm long
PA-DIA/025	185mm long
PA-DIA/026	228mm long

Curved

Code	Description
PA-DIA/019	152mm long
PA-DIA/020	178mm long
PA-DIA/021	185mm long
PA-DIA/022	228mm long

Did you know...

The difference between Monopolar Electrosurgery and Bipolar Electrosurgery


There is one basic difference between bipolar and monopolar techniques. With monopolar electrosurgery, a probe electrode is used to apply the electrosurgical energy to the target tissue to achieve the desired surgical effect. The current then passes through the patient to a return pad and then back to the ESU generator to complete the circuit.

With the bipolar electrosurgical method a bipolar device, often a set of forceps, is used. The electrical current passes from one side of the forcep, through the target tissue to the other side of the forcep, then back to the generator. The electrical current is restricted to the tissue between the forcep, therefore not requiring the use of a grounding pad.

Bipolar Forceps

Bipolar Forceps

Straight

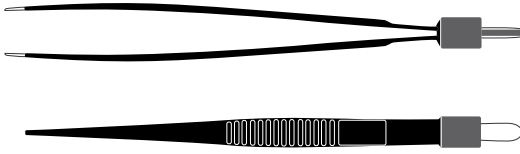

Fine tip

Code	Description
PA-DIA/034	101mm long
PA-DIA/035	127mm long
PA-DIA/036	152mm long
PA-DIA/037	178mm long
PA-DIA/038	185mm long

Medium tip


Code	Description
PA-DIA/039	101mm long
PA-DIA/040	127mm long
PA-DIA/041	152mm long
PA-DIA/042	178mm long
PA-DIA/043	185mm long

Heavy tip

Code	Description
PA-DIA/044	101mm long
PA-DIA/045	127mm long
PA-DIA/046	152mm long
PA-DIA/047	178mm long
PA-DIA/048	185mm long

Bipolar Forceps

Angled

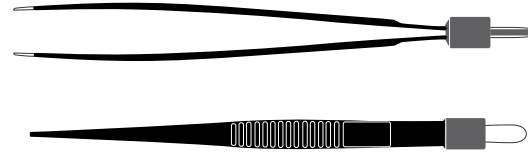

Fine tip

Code	Description
PA-DIA/049	101mm long
PA-DIA/050	127mm long
PA-DIA/051	152mm long
PA-DIA/052	178mm long
PA-DIA/053	185mm long

Medium tip

Code	Description
PA-DIA/054	101mm long
PA-DIA/055	127mm long
PA-DIA/056	152mm long
PA-DIA/057	178mm long
PA-DIA/058	185mm long

Heavy tip

Code	Description
PA-DIA/059	101mm long
PA-DIA/060	127mm long
PA-DIA/061	152mm long
PA-DIA/062	178mm long
PA-DIA/063	185mm long

Adson Bipolar Forceps




Code	Description
PA-DIA/003a	152mm long

Need Single Use Instruments?

Order your copy of Surgical Holdings Single Use Solutions brochure Light Sticks

- Symmetry Surgical
- Electrosurgery
- Single Use Forceps

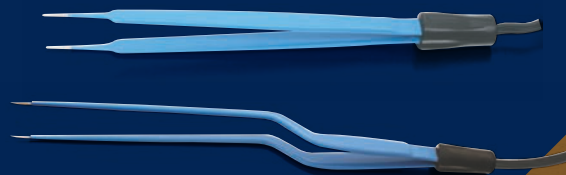

Better Availability



Great Range of Products



Perfect Condition, Every Time


Handles, Needles and Blades

Monel Handle



Code	Description
PA-DIA/028	145mm long

Monel Blade




Code	Description
PA-DIA/029	Fully insulated
PA-DIA/030	Non-insulated

Needle Handles



Code
PA-DIA/027

Needles

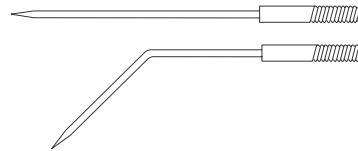


Straight

Code	Description
PA-DIA/064	Stout
PA-DIA/064a	Medium

Angled

Code	Description
PA-DIA/064b	Stout
PA-DIA/064c	Medium

Abbey Diathermy Needle

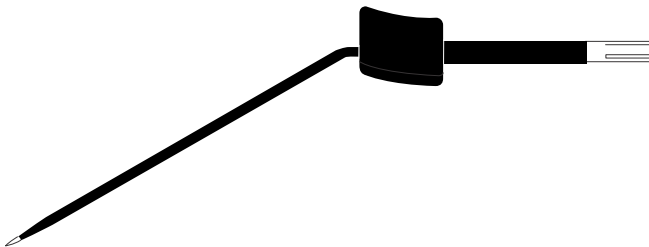

Code
PA-DIA/078

Diathermy Arm

With ball



Code	Description
PA-DIA/069	Curved
PA-DIA/069a	Straight

Finger Switch Pencil

With spatula and 3 metre lead



Code
PA-DIA/068

Spatula Blade

For diathermy finger



Code
PA-DIA/067a

Needle Point


For diathermy finger



Code
PA-DIA/067b


Leads and Quivers

Leads

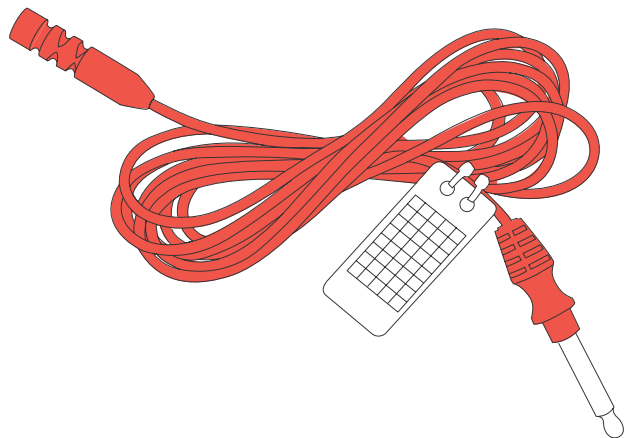

Code	Description
PA-DIA/065	4mm plug end
PA-DIA/066	8mm plug end


Bipolar Leads

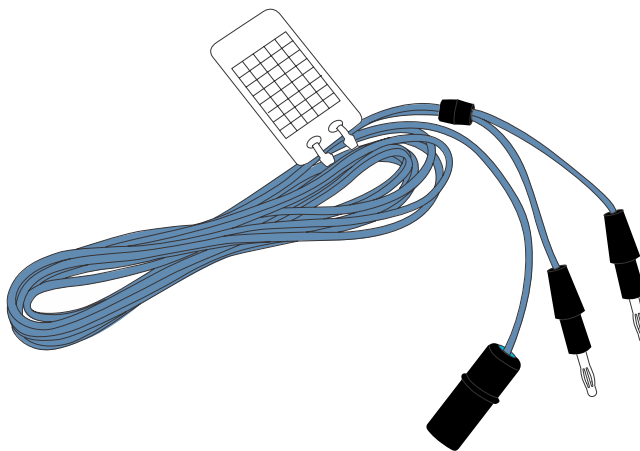

Code	Description
PA-DIA/067	Standard

Quiver


With hole in end, 232mm long

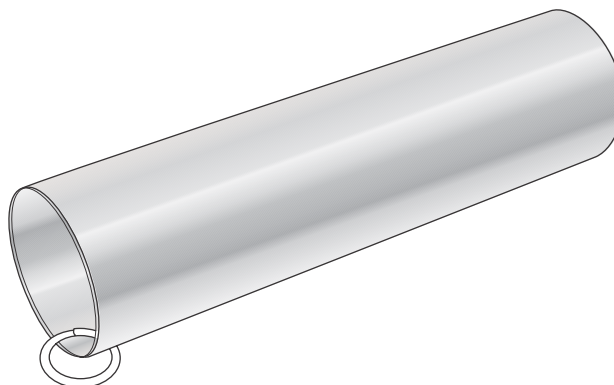

Code	Description
PA-DIA/001	Standard

Quiver

With hole in end, 232mm long

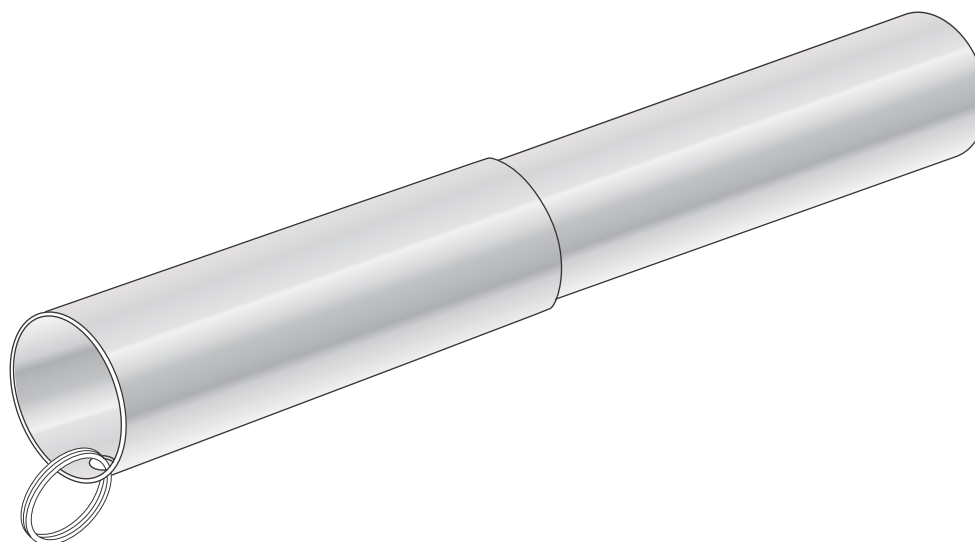

Code	Description
PA-DIA/002	Telescopic




CONTACT US

 +62 856-6381-381

 inquiry@averonindonesia.com

 sales@averonindonesia.com

 www.averonindonesia.com

 Axa tower - Kuningan City Lt 45-7A Jl Prof. DR. Satrio, Kuningan, Kecamatan Setiabudi, Kota Jakarta Selatan, Daerah Khusus Ibukota Jakarta 12940.